IB/2005/050072

PA 1257060

THE UNITED STATES OF AMERICA

TO ALL TO WHOM THESE PRESENTS SHALL COME:

UNITED STATES DEPARTMENT OF COMMERCE

United States Patent and Trademark Office

December 09, 2004

THIS IS TO CERTIFY THAT ANNEXED HERETO IS A TRUE COPY FROM THE RECORDS OF THE UNITED STATES PATENT AND TRADEMARK OFFICE OF THOSE PAPERS OF THE BELOW IDENTIFIED PATENT APPLICATION THAT MET THE REQUIREMENTS TO BE GRANTED A FILING DATE UNDER 35 USC 111.

APPLICATION NUMBER: ***60/536,757***
FILING DATE: ***January 15, 2004***

PRIORITY DOCUMENT
SUBMITTED OR TRANSMITTED IN COMPLIANCE WITH RULE 17.1(a) OR (b)

By Authority of the
COMMISSIONER OF PATENTS AND TRADEMARKS

L. Edelen

L. EDELEN
Certifying Officer

22783 U.S. PTO

Please type a plus sign (+) inside this box → +

PTO/SB/16 (02-01)
Approved for use through 10/31/2002. OMB 0651-0032
Patent and Trademark Office; U.S. DEPARTMENT OF COMMERCE
Under the Paperwork Reduction Act of 1995, no persons are required to respond to a collection of information unless it displays a valid OMB control number.

PROVISIONAL APPLICATION FOR PATENT COVER SHEET

This is a r quest for filing a PROVISIONAL APPLICATION FOR PATENT under 37 CFR 1.53 (c).

Express Mail Label No. EL998016713US

INVENTOR(S)		
Given Name (first and middle [if any])	Family Name or Surname	Residence (City and either State or Foreign Country)
Anne	NIEMI	HELSINKI, FINLAND
Jukka	TANTTU	ESPOO, FINLAND

☒ *Additional inventors are being named on the ONE separately numbered sheets attached hereto*

TITLE OF THE INVENTION (280 characters max)

COIL SENSITIVITY ESTIMATION FOR PARALLEL IMAGING

CORRESPONDENCE ADDRESS

Direct all correspondence to:

☐ Customer Number → *Place Customer Number Bar Code Label here*

OR *Type Customer Number here*

15535 U.S. PTO 60/536757 011504

☒ Firm *or* Individual Name	THOMAS E KOCOVSKY, JR				
Address	FAY, SHARPE, FAGAN, MINNICH & McKEE, LLP				
Address	1100 SUPERIOR AVENUE, SEVENTH FLOOR				
City	CLEVELAND	State	OH	ZIP	44114
Country	US	Telephone	216/861-5582	Fax	216/241-1666

ENCLOSED APPLICATION PARTS *(check all that apply)*

☒ Specification *Number of Pages* 11 ☐ CD(s), Number

☒ Drawing(s) *Number of Sheets* 3 ☐ Other (specify)

☒ Application Data Sheet. See 37 CFR 1.76

METHOD OF PAYMENT OF FILING FEES FOR THIS PROVISIONAL APPLICATION FOR PATENT *(check one)*

☐ Applicant claims small entity status. See 37 CFR 1.27.

☒ A check or money order is enclosed to cover the filing fees

☒ The Commissioner is hereby authorized to charge filing fees or credit any overpayment to Deposit Account Number: 06-0308

☐ Payment by credit card. Form PTO-2038 is attached.

FILING FEE AMOUNT ($) 160

The invention was made by an agency of the United States Government or under a contract with an agency of the United States Government.

☐ No.

☐ Yes, the name of the U.S. Government agency and the Government contract number are: _____.

Respectfully submitted,
SIGNATURE Thomas E. Kocovsky

Date 01/15/2004

TYPED or PRINTED NAME Thomas E. KOCOVSKY, Jr

REGISTRATION NO. 28,383 *(if appropriate)*

Docket Number: PHUS040040USP

TELEPHONE 216 861-5582

USE ONLY FOR FILING A PROVISIONAL APPLICATION FOR PATENT

This collection of information is required by 37 CFR 1.51. The information is used by the public to file (and by the PTO to process) a provisional application. Confidentiality is governed by 35 U.S.C. 122 and 37 CFR 1.14. This collection is estimated to take 8 hours to complete, including gathering, preparing, and submitting the complete provisional application to the PTO. Time will vary depending upon the individual case. Any comments on the amount of time you require to complete this form and/or suggestions for reducing this burden, should be sent to the Chief Information Officer, U.S. Patent and Trademark Office, U.S. Department of Commerce, Washington, D.C., 20231. DO NOT SEND FEES ORCOMPLETED FORMSTO THIS ADDRESS. SEND TO: Box Provisional Application, Assistant Commissioner for Patents, Washington, D.C. 20231.

PROVISIONAL APPLICATION COVER SHEET
Additional Page

Docket Number	PHUS040040USP	Type a plus sign (+) inside this box →	+

INVENTOR(S)/APPLICANT(S)		
Given Name (first and middle [if any])	Family or Surname	Residence (City and either State or Foreign Country)
Mika	YLIHAUTALA	VANTAA, FINLAND

Number ONE of ONE

WARNING: Information on this form may become public. Credit card information should not be included on this form. Provide credit card information and authorization on PTO-2038.

COIL SENSITIVITY ESTIMATION FOR PARALLEL IMAGING

Background of the Invention

The following relates to the diagnostic imaging arts. It finds particular application in reducing artifacts in magnetic resonance parallel imaging techniques.

In magnetic resonance imaging apparatus used for medical diagnostics of the human body, the body axis is usually oriented along a horizontal x-axis of a rectangular coordinate system. The body region to be examined is situated between the pole pieces of a magnet, which generates a temporally constant main magnetic field, B_0, extending along a vertical or z-axis. A resonator is provided for transmitting the excitation signals and receiving the resonance signals. When a substance such as human tissue is subjected to the uniform magnetic field, B_0, the individual magnetic moments of the spins in the tissue preferentially align with this polarizing field. If the substance, or tissue, is subjected to an excitation radio frequency field, B_1, which is in the x-y plane and which is near a characteristic Larmor frequency, the net aligned moment, M_z, precesses about the z-axis to produce a net transverse magnetic moment, M_t. A resonance signal is emitted by the excited spins after the excitation signal B_1 is terminated. This signal may be received and processed to form an image.

When utilizing these signals to produce images, magnetic field gradients, G_x, G_y and G_z, are employed to provide spatial encoding of the resonance signal along x, y, and z axes, respectively. Typically, the region to be imaged is scanned by a sequence of measurement cycles in which these gradients vary according to the particular localization method being used. The resulting set of received NMR signals are digitized and processed to reconstruct the image using one of many well known reconstruction techniques.

One method of acquiring an NMR data set from which an image can be reconstructed employs a variable amplitude phase encoding magnetic field gradient pulse prior to the acquisition of NMR spin-echo signals to phase encode spatial information in the direction of the gradient. In a two-dimensional implementation (2DFT), for example, spatial information is encoded in one direction by applying a phase encoding gradient pulse, G_y, prior to each gradient echo signal which is acquired in the presence of a readout magnetic field gradient G_x, in a direction orthogonal to the phase encoding direction. The readout gradient present during the spin-echo acquisition also encodes spatial information in a direction orthogonal to the phase encoding gradient. Rather than generating a series

of contiguous 2D slice images, a 3D image can be generated by phase encoding along the desired axis. Each echo produces data along a trajectory or line in k-space. Data sets in k-space are inverse Fourier transformed or otherwise reconstructed into image space. The acquisition of each phase encoded data line requires a finite amount of time, and the more data that are required to obtain an image of the prescribed field of view (FOV) and spatial resolution, the longer the total scan time.

Many technical developments in the field of MR imaging aim to reduce data acquisition time. One such development is known as parallel imaging, in which images are acquired with sub-sampled signal acquisitions resulting in fold-over artifacts. The fold-over may be removed by a sensitivity encoding (SENSE) technique. The folded images reconstructed from each coil are combined using the receive coil sensitivities of multiple receive coils with different sensitivity characteristics to unfold the fold-over artifacts. This technique is described by K. P. Pruessmann, et al., "SENSE: Sensitivity Encoding for Fast MRI", Magnetic Resonance in Medicine 42, 952-962 (1999). The coil sensitivities are estimated from a calibration image scanned with full field-of-view.

Rapid magnetic field changes, occurring at the edges of the homogeneous main magnetic field, or when magnetic materials are introduced in or near to the imaging volume, result in image distortions both in the calibration and the actual acquisition. These distortions appear as abrupt magnitude and phase variations that depend on the acquisition parameters.

In parallel imaging reconstruction, distortions in the sensitivity calibration may result in a failure of the unfolding procedure, which appear as fold-over like artifacts that disrupt the final image quality. The artifacts are more likely to be seen if the image distortions of the calibration sequence and the actual sequence deviate from each other. For example, in a gradient recalled echo image there may be curled and striped artifacts, whereas in a fast spin echo image bright curved stripes may be seen.

The present invention contemplates an improved method and apparatus that overcomes the aforementioned limitations and others.

Brief Summary of the Invention

It is an object of the present invention to provide an improved method of coils' sensitivity estimation for parallel imaging in order to provide improved image quality with a reduction in the number and magnitude of visible artifacts.

According to one aspect, a method of improved coil sensitivity estimation is provided for reducing artifacts in an MRI apparatus utilizing parallel imaging. The method includes performing a calibration sequence in relation to an imaging sequence and using either a spin echo type sequence for each calibration or a gradient recalled echo sequence with a short echo time for each calibration, and matching the phase encode direction of the calibration scan and the parallel imaging scan.

According to another aspect, an MRI apparatus is provided that includes a magnet system for generating a B_0 magnetic field in an examination zone. The apparatus includes a means for exciting and manipulating magnetic resonance in the examination zone and a means for spatially encoding the magnetic resonance. Also provided is a plurality of coils with differing sensitivity profiles for receiving resonance signals in parallel and a means for reconstructing received resonance signals into image representations. Another means generates sensitivity profiles of the coils from image representations generated during a calibration scan. Still another means generates a diagnostic image from the sensitivity profiles and image representations generated during a diagnostic scan. A sequence control means for accessing a calibration sequence memory means to retrieve either an RF refocused spin echo type sequence or a gradient recalled echo type sequence, and controlling the resonance exciting means and the spatial encoding means in accordance with the retrieved calibration sequence to generate resonance signals for the reconstruction means to reconstruct into the calibration image representations. It accesses a diagnostic imaging sequence memory means to retrieve a diagnostic imaging sequence and controls the resonance exciting means and the spatial encoding means to generate resonance signals for the reconstruction means to reconstruct into the diagnostic image representations.

One advantage resides in a reduction of magnitude, phase and position errors occurring in a calibration scan.

A still further improvement resides in the reduced or removed image fold-over artifacts in parallel imaging.

Another advantage resides in the improved image quality.

Numerous additional advantages and benefits will become apparent to those of ordinary skill in the art upon reading the following detailed description of the preferred embodiments.

Brief Description of the Drawings

The invention may take form in various components and arrangements of components, and in various process operations and arrangements of process operations.

The drawings are only for the purpose of illustrating preferred embodiments and are not to be construed as limiting the invention.

FIGURE 1 diagrammatically shows a magnetic resonance imaging system constructed according to the concepts of the present invention;

FIGURE 2 shows a representation of an MRI image without SENSE acquired using a gradient recalled echo type sequence;

FIGURE 3 shows a representation of a SENSE image corresponding to the image of FIGURE 2 acquired using a gradient recalled echo based calibration where the phase encode direction of the parallel imaging scan and the calibration scan are orthogonal;

FIGURE 4 shows a representation of a SENSE image corresponding to the image of FIGURE 2 acquired using a spin echo based calibration where the phase encode direction of the parallel imaging scan and the calibration scan coincide, and the read-out gradients of these two scans are essentially the same in magnitude and direction;

FIGURE 5 shows a representation of an MRI image without SENSE acquired using a fast spin echo type sequence;

FIGURE 6 shows a representation of a SENSE image corresponding to the image of FIGURE 5 acquired using a gradient recalled echo based calibration where the phase encode direction of the parallel imaging scan and the calibration scan are orthogonal; and

FIGURE 7 shows a representation of a SENSE image corresponding to the image of FIGURE 5 acquired using a spin echo based calibration where the phase encode direction of the parallel imaging scan and the calibration scan coincide, and the read-out gradients of these two scans are essentially the same in magnitude and direction. This results in the same signal bandwidth per unit length in both scans, and the B_0 errors create the same position error measured in mm's. The data sampling time–and thus the resolution in read out direction–of the two scans may differ.

Detailed Description of the Preferred Embodiments

With reference to FIGURE 1, a magnetic resonance imaging apparatus **40** includes a main magnet **42** system for generating a temporally constant B_0 magnetic field that extends vertically in an examination zone in the z direction of an xyz coordinate system as shown. A region of interest of a patient **44** is disposed in an examination zone **46** defined by the FOV of the apparatus—often a spherical region. The magnet system includes a ferrous yoke defining a flux return path between pole pieces **48,50**. Coil windings, superconducting or resistive, are disposed adjacent the pole pieces **48,50** or along the flux return path. Alternately, the yoke can be a permanent magnet.

Gradient coil systems **52,54** generate spatially variant magnetic field pulses with an approximately linear gradient in the x direction, the y direction or the z direction. A respective resonator **56,58** that is resonant at the Larmor frequency of a selected dipole, e.g. H^1, is disposed between each gradient coil system **52,54** and the examination zone. An RF shielding screen **60** is disposed between the resonators and the gradient coils. The resonators **56,58** and RF shields **60,62**, are arranged in a mirror-image fashion relative to the examination zone. Each resonator **56,58** preferably functions as a transmit coil, but may also be operative as a receive coil.

A sequence control processor **70** controls a radio frequency transmitter **72a** associated with the transmit/receive body coils **56,58** and a gradient field controller **72b** to induce and manipulate spatially encoded resonance as known in the art. More specifically, during generation of a calibration image, the sequence control accesses a calibration sequence memory **74** to retrieve a spin-echo, fast spin echo, or similar sequence in which the phase of the excited resonance is refocused with an RF-pulse. A gradient recalled echo with a very short echo time, e.g. less than 5 msec, is also suitable for calibration.

During the calibration scan, the generated magnetic resonance signals are picked up by a plurality of SENSE coils **76a,76b,...,76n** and demodulated by corresponding receivers **78a,78b,...,78n**. The resonance signals may also be received by the resonators **56,58** operating in a receive mode and demodulated by a receiver **78o**. The resonance data from each of the SENSE coils and the resonators is individually reconstructed **80a,80b,...,80n,80o** into a plurality of SENSE images stored in SENSE image memory sectors **82a,82b,...,82n** and a reference image stored in reference image memory sector **82o**. A calibration processor **84** compares the SENSE images and the reference image to generate sensitivity profiles for the SENSE coils, which are stored in a sensitivity map memory **86**.

For final imaging, the sequence control **70** accesses a diagnostic imaging sequence memory **88** to select an imaging sequence. The resonance signals are received by the SENSE coils **76a,...,76n**, demodulated by receivers **78a,...,78n**, and reconstructed **80a,...,80n** into a series of under-sampled, folded images **82a,...,82n**. A SENSE processor **90** combines and unfolds the SENSE images in accordance with the sensitivity profile information from the sensitivity map memory **86** to generate a final 3D image for storage in a final image memory **92**. An image processor **94** selects and formats portions of the image data for display on a monitor **96**.

In the above-described SENSE imaging, the calibration sequence is conducted in order to generate sensitivity profiles or maps of each of the SENSE coils. This calibration

scan is typically conducted using field echoes. However, the present inventors have found that when the calibration sequence is used on open scanners, artifacting and errors may occur. Specifically, they have determined that in the open system, the B_0 magnetic field rolls over relatively gradually at the edge of the field of view. The presence of this strong magnetic field variation outside of the field of view causes magnitude, phase and position errors in the calibration scan. Especially it shall be noted that the main field variations create position errors more easily in the read-out direction than in the phase encoding direction.

Coil sensitivity information can be accurately estimated in the regions of the main magnetic field where the above-described distortions appear. This is accomplished by performing the coil sensitivity estimation with a calibration sequence that reduces the phase and magnitude distortions to an equal or smaller level than in the actual parallel imaging scan. The position distortions in the two images shall be about the same.

The inventors have found that by conducting a calibration scan using spin-echo type sequences, this problem can be cured. The refocusing pulse for the spin-echo also refocuses the phase errors, effectively canceling them at the spin echo. Alternatively, a gradient echo based calibration can be used if the echo time is made very small to minimize the accumulated phase errors. Because the errors appear differently in the phase and read directions, the differences between the calibration and SENSE imaging scans are smaller when the phase encode direction(s) in the calibration and SENSE scans are both in the same direction. A still further improvement is provided if the readout gradient direction and magnitude are essentially the same in both the calibration and the SENSE imaging scans.

It is not required that the slice positions of the calibration and diagnostic scan should be exactly the same. It is required that the calibration scan should cover at least the same imaging volume as the diagnostic scan. The coil sensitivity maps for each slice position of the diagnostic scan can be obtained with interpolation.

With reference to FIGURE 2, a representation is shown of a first image **10** acquired without SENSE, done with a gradient recalled echo (GRE) type sequence on an open MRI system. With reference now to FIGURE 3, a second GRE image **12** of the same subject as used for the first GRE image **10** is shown. However, this image was acquired using SENSE with gradient recalled echo based calibration as known in the previous art. In the second GRE image, curled and striped fold-over artifacts **14,16,** arising from the incomplete unfolding reconstruction due to errors in the sensitivity calibration, are clearly evident when compared to the first image **10.**

With reference now to FIGURE 4, a third GRE image **18** acquired according to an embodiment of the present invention is shown. In this embodiment, the coil sensitivity estimation is performed with a spin echo type calibration sequence where the phase encode direction of the parallel imaging scan and the calibration scan coincide, and the sampling bandwidth per unit length in the read-out direction of these two scans are the same. Curled and striped artifacts **20,22** in the third image **18** are clearly reduced when compared to the artifacts **14,16** of the second image **12**. The images of FIGURES 2-4 were all acquired with a repetition time (TR) of 40 ms, an echo time (TE) of 10 ms, a slice thickness of 10 mm, a number of excitations (NEX) of 2, a FOV of 550 mm, a 256x256 matrix, phase encoding in the vertical direction, and a bandwidth (BW) of 62.5 Hz/pixel.

FIGURES 5-7 show a sequence of images acquired in a fashion similar to the images **10,12,18** of FIGURES 2-4 but acquired using a fast spin echo (FSE) type sequence. With reference to FIGURE 5, a representation is shown of a first FSE image **24** acquired without SENSE. With reference now to FIGURE 6, a second FSE image **26** of the same subject as used for the first FSE image **24** is shown. This image was acquired using SENSE with gradient recalled echo based calibration and shows curled and striped artifacts **28,30** when compared to the first image **24**.

With reference now to FIGURE 7, a third FSE image **32** was acquired in a manner similar to the second FSE image **26**, however, a spin echo based calibration was utilized in place of the gradient recalled echo based calibration. Also the phase encode direction of the parallel imaging scan and the calibration scan coincide, and the sampling bandwidth per unit length in the read-out direction of these two scans are the same. Curled and striped artifacts **34,36** in the third FSE image are clearly reduced when compared to the artifacts **28,30** of the second FSE image. The images of FIGURES 5-7 were all acquired with a TR of 410 ms, a TE of 20 ms, a slice thickness of 3.0 mm, a NEX of 3, a FOV of 550 mm, a 288x288 matrix, phase encoding in the vertical direction, and a BW of 71.4 Hz/pixel.

The invention has been described with reference to a preferred embodiment. The invention has also been described with respect to several alternate embodiments. For example, the invention is not limited to open MR scanners but is valid for any type of magnet configuration, including bore type scanners. Neither is the generation of a reference image with the described transmit/receive body coils **56, 58** necessary, since the reference image can be calculated from a combination image using SENSE coils **76a, 76b,...,76n**. These and other variations and modifications of the invention will occur to others upon the reading and understanding of this specification. It is intended that all such

variations, alterations and modifications, be included insofar as they come within the scope of the appended claims or the equivalents thereof.

Claims

Having thus described the system embodiments the invention is now claimed to be:

1. A method of improved coil sensitivity estimation for reducing artifacts in an MRI apparatus utilizing parallel imaging, the method comprising:

for a parallel imaging sequence, performing a calibration sequence relative to the parallel imaging sequence, using one of:

a spin echo type sequence matching the in-plane phase encode direction of the calibration and the parallel imaging sequences for each calibration; and

a gradient echo type sequence matching the in-plane phase encode direction of the calibration and the parallel imaging sequences for each calibration.

2. The method as set forth in claim 1, wherein the calibration sequence is performed for each parallel imaging sequence.

3. The method as set forth in claim 2, wherein the calibration sequence is performed prior to each said parallel imaging sequence.

4. The method as set forth in claim 1, wherein the gradient echo type calibration sequence is performed with a very short echo time (TE), e.g. less than 5 ms.

5. The method as set forth in claim 1, further including:

using an essentially identical read out gradient in both the calibration sequence and the parallel imaging sequence.

6. The method according to claim 1, wherein a phase encode direction of said calibration sequence is essentially directed in along a phase encode direction of said parallel imaging sequence.

7. An MRI apparatus having a sequence controller (70) programmed to perform the method as set forth in any of claims 1-6.

8. An MRI apparatus that includes a magnet system for generating a B_0 magnetic field in an examination zone (46), the apparatus comprising:

means **(58,72a,76a,...,76n)** for exciting and manipulating magnetic resonance in the examination zone;

means **(52,74,72b)** for spatially encoding the magnetic resonance;

plurality of coils **(76a,...,76n)** with differing sensitivity profiles for receiving resonance signals in parallel;

means **(80a,...,80o)** for reconstructing received resonance signals into image representations;

means **(84)** for generating sensitivity profiles **(86)** of the coils **(76a,...,76n)** from image representations **(82a,...,82n)** generated during a calibration scan;

means **(90)** for generating a diagnostic image **(92)** from the sensitivity profiles **(86)** and image representations **(82a,...,82n)** generated during a diagnostic scan;

sequence control means **(70)** for accessing a calibration sequence memory means **(74)** to retrieve one of an RF refocused spin echo type sequence and a gradient recalled echo type sequence and controlling the resonance exciting means **(58,72a,76a,...,76n)** and the spatial encoding means **(52,74,72b)** in accordance with the retrieved calibration sequence to generate resonance signals for the reconstruction means **(80a,...,80o)** to reconstruct into the calibration image representations **(82a,...,82n)** and for accessing a diagnostic imaging sequence memory means **(88)** to retrieve a diagnostic imaging sequence and controlling the resonance exciting means **(58,72a,76a,...,76n)** and the spatial encoding means **(52,74,72b)** to generate resonance signals for the reconstruction means **(80a,...,80o)** to reconstruct into the diagnostic image representations **(82a,...,82n)**.

ABSTRACT

In a parallel or SENSE imaging technique in an MRI system **(40)**, a calibration scan is conducted to generate a calibration image **(86)** indicative of sensitivity profiles of parallel imaging coils **(76a,...,76n)** also in the regions where the magnetic field is distorted. This is accomplished by using a phase refocusing imaging protocol such as a spin echo technique, or by using a gradient echo technique where the echo time is very short. In addition, the phase encode direction of the calibration scan and a diagnostic imaging scan shall be matched. A diagnostic imaging scan is conducted using a diagnostic scan protocol to generate a diagnostic image representation from each parallel imaging coil. A SENSE processor **(90)** reconstructs a final diagnostic image **(92)** from the diagnostic image representations and the coil sensitivity profiles.

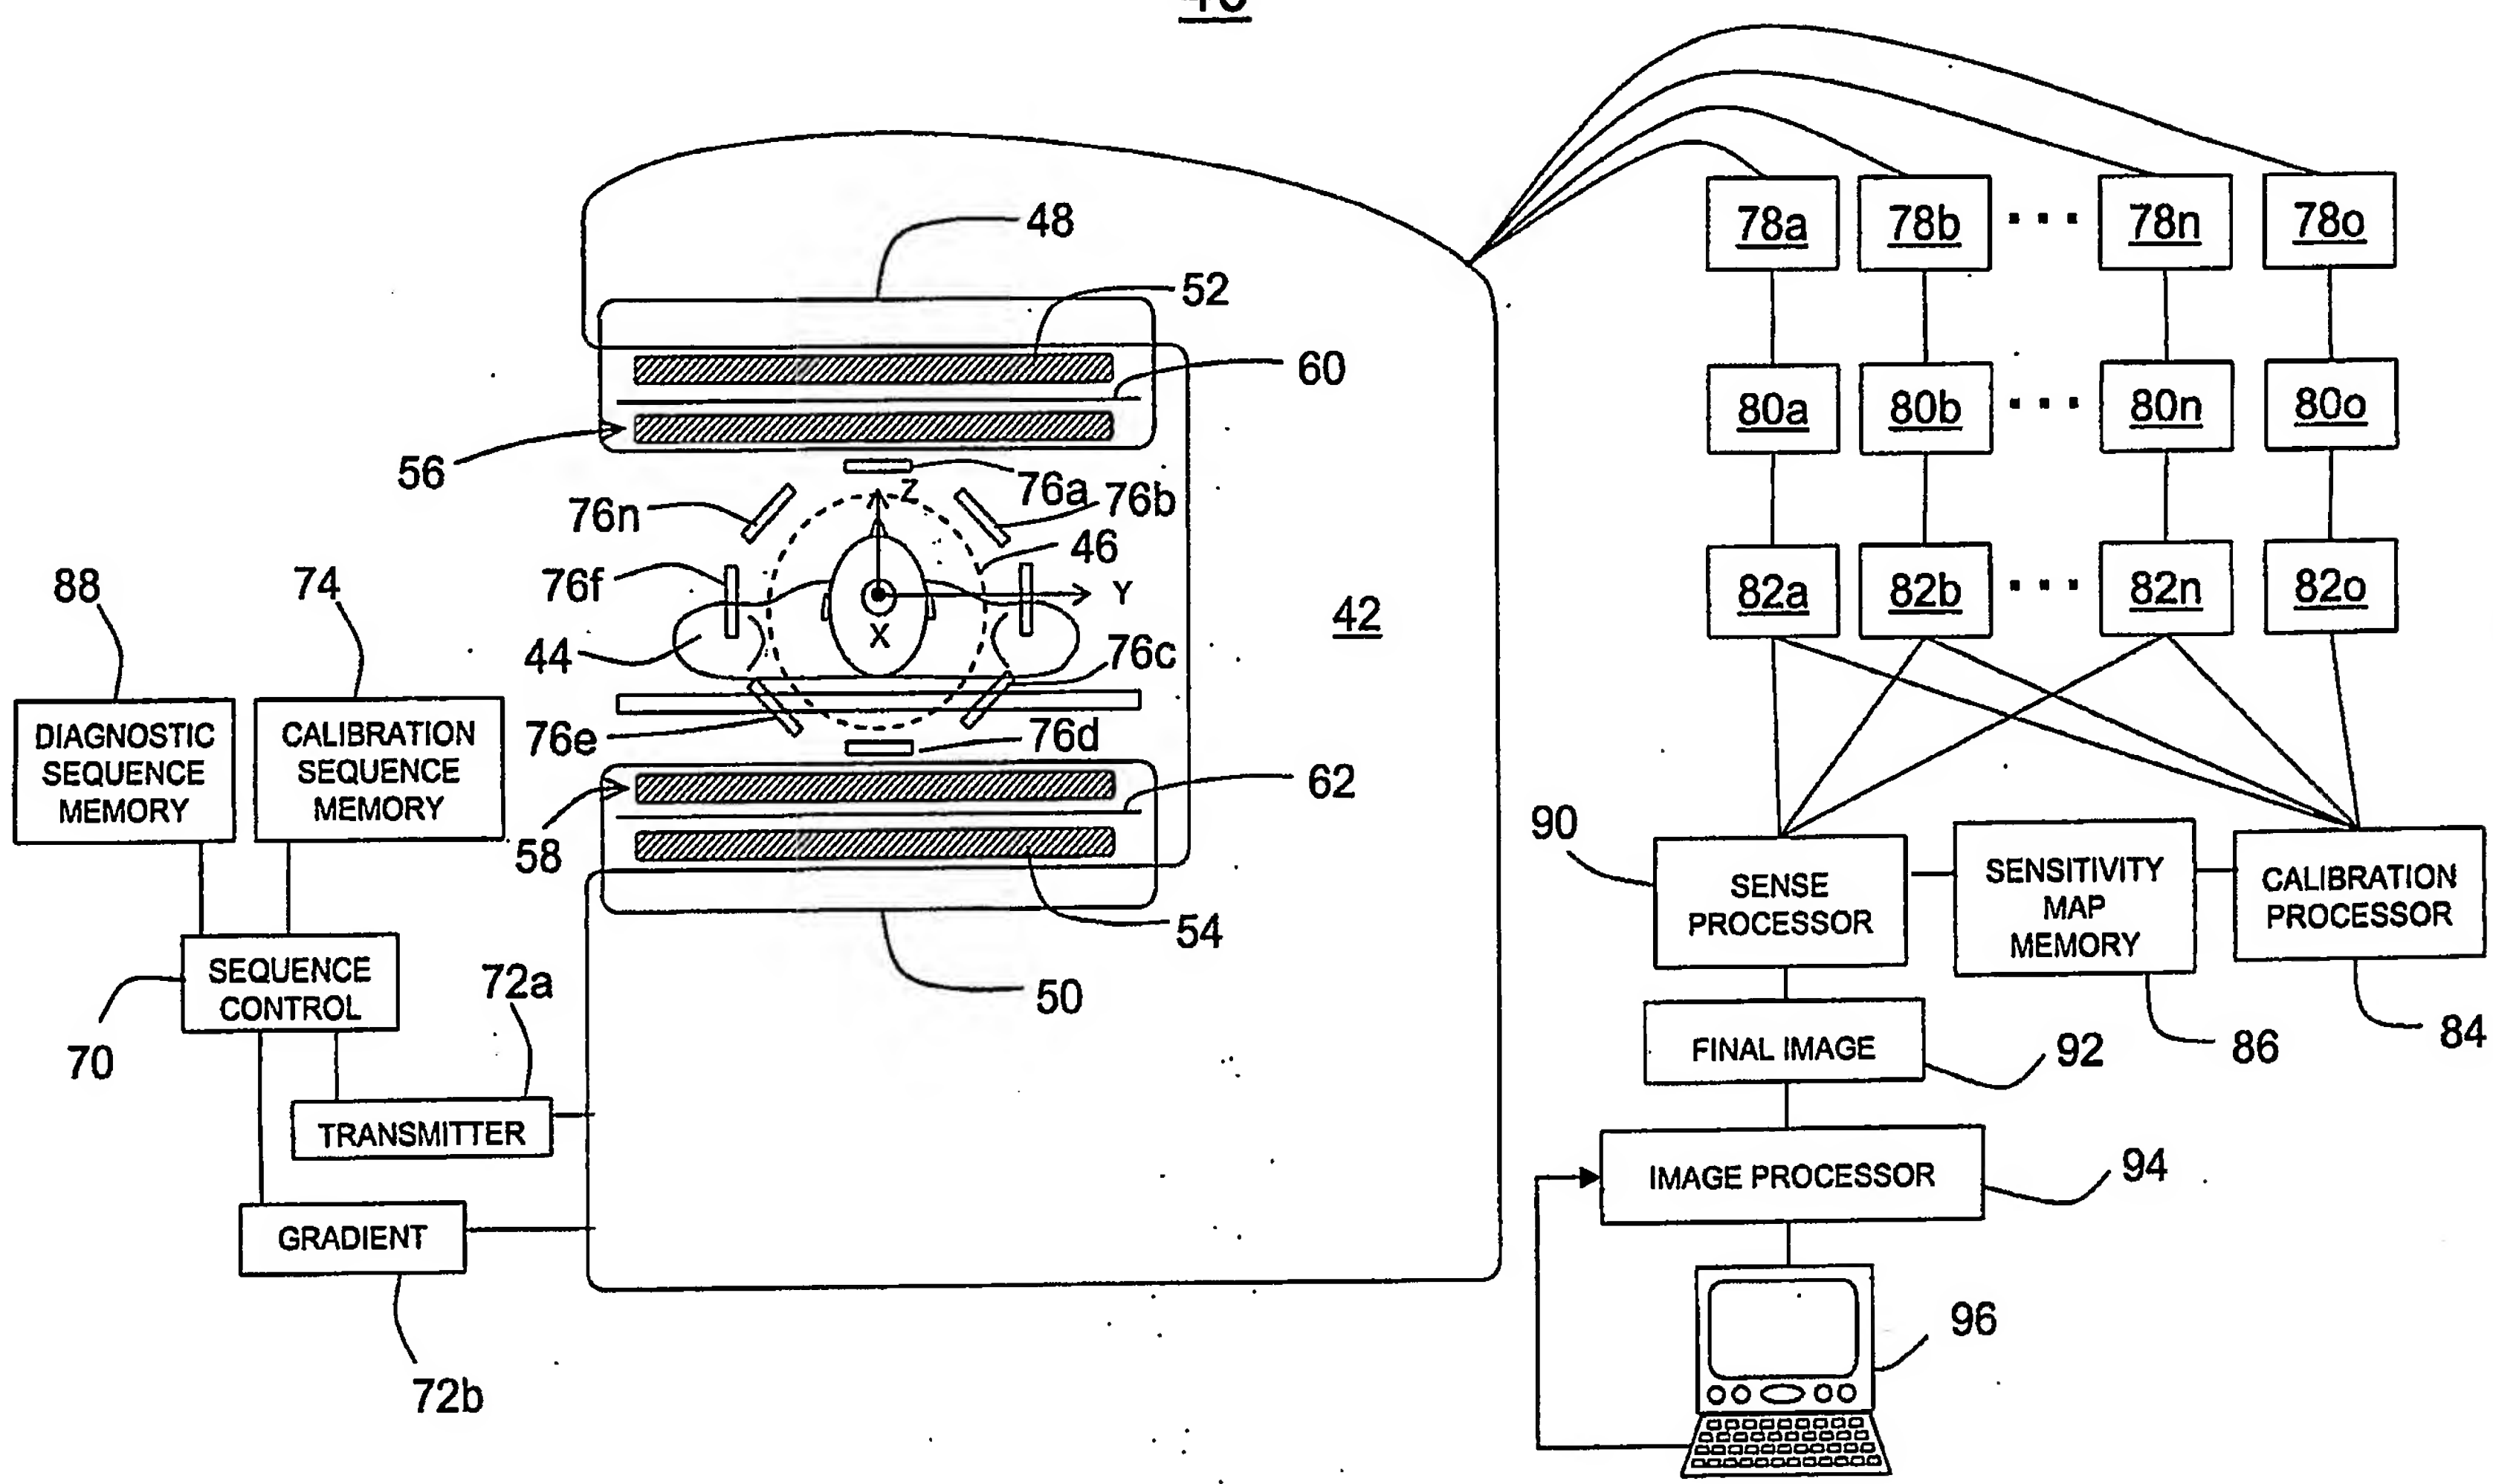
40
48
52
60
56
76n
76a
76b
Z
46
Y
X
76f
44
76c
42
76e
76d
62
58
54
50
88
DIAGNOSTIC SEQUENCE MEMORY
74
CALIBRATION SEQUENCE MEMORY
SEQUENCE CONTROL
70
72a
TRANSMITTER
GRADIENT
72b
78a
78b
78n
78o
80a
80b
80n
80o
82a
82b
82n
82o
90
SENSE PROCESSOR
SENSITIVITY MAP MEMORY
CALIBRATION PROCESSOR
FINAL IMAGE
92
86
84
IMAGE PROCESSOR
94
96

FIG 1

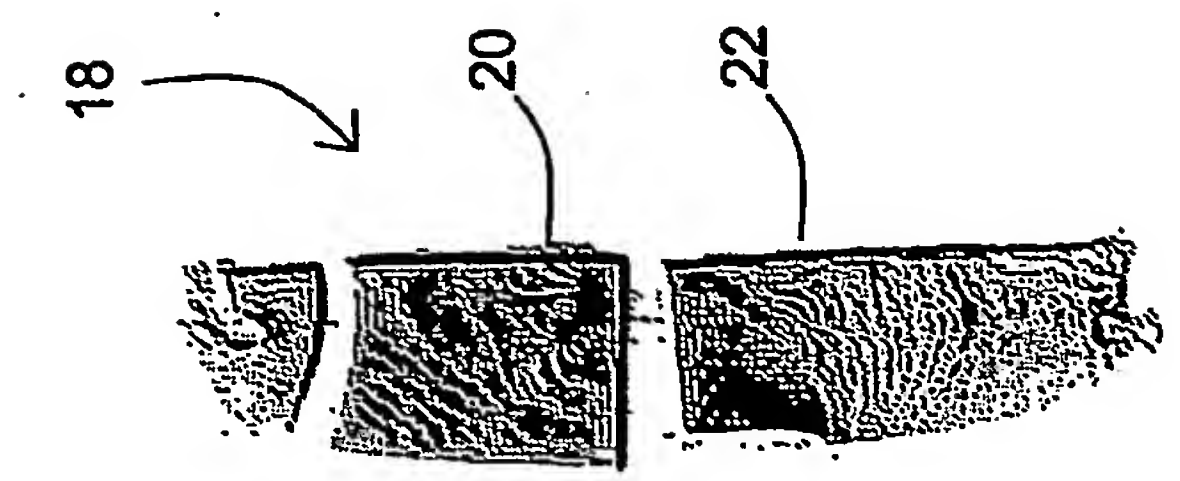

FIG 4

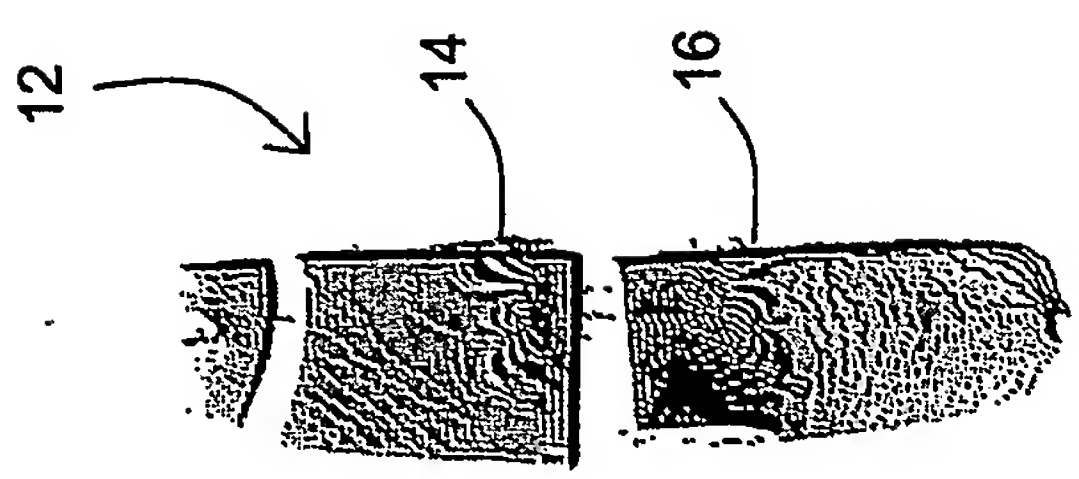

FIG 3

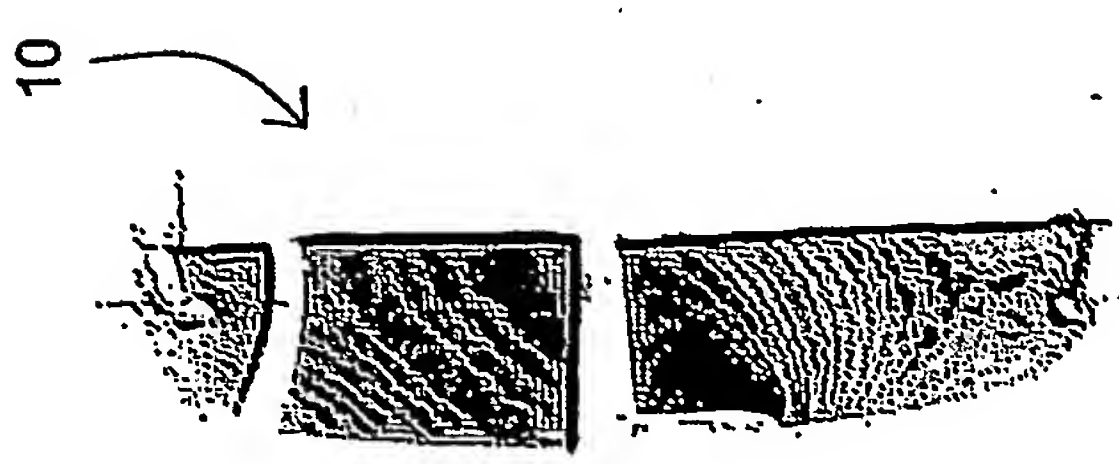

FIG 2

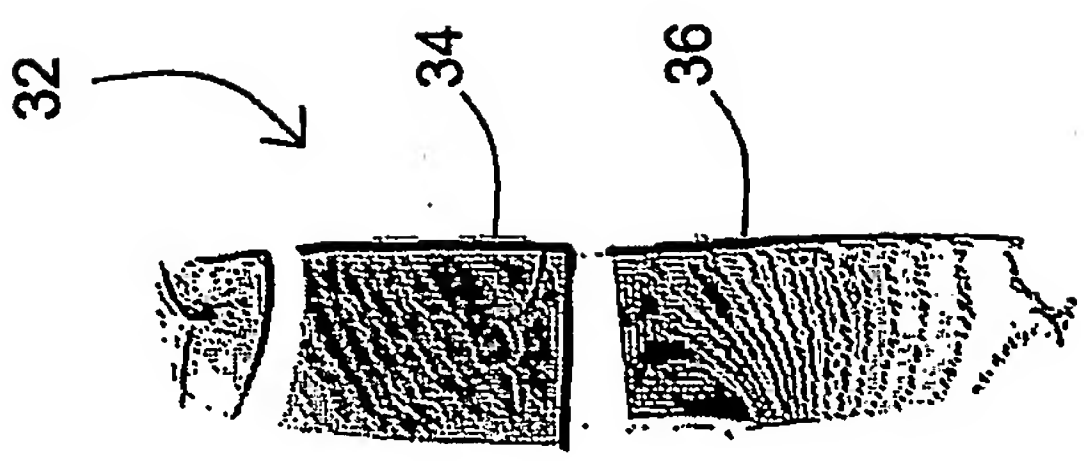

FIG 7

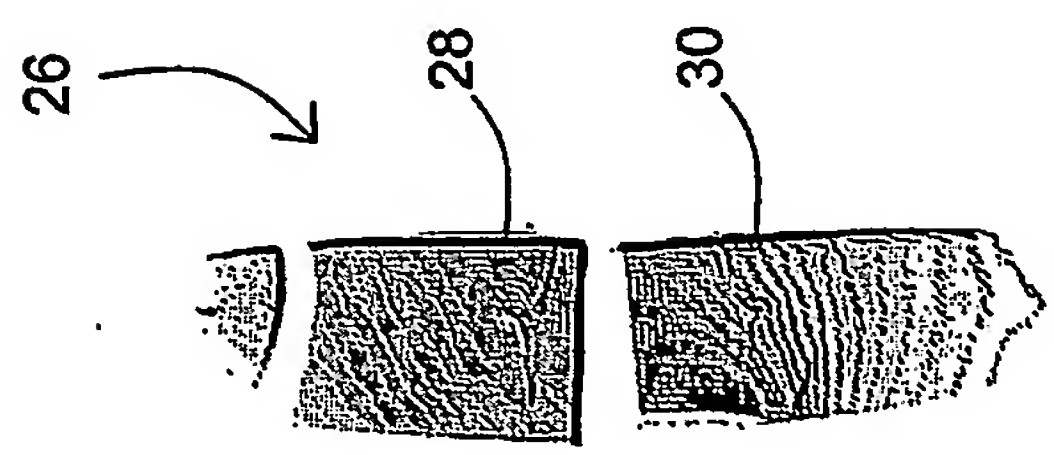

FIG 6

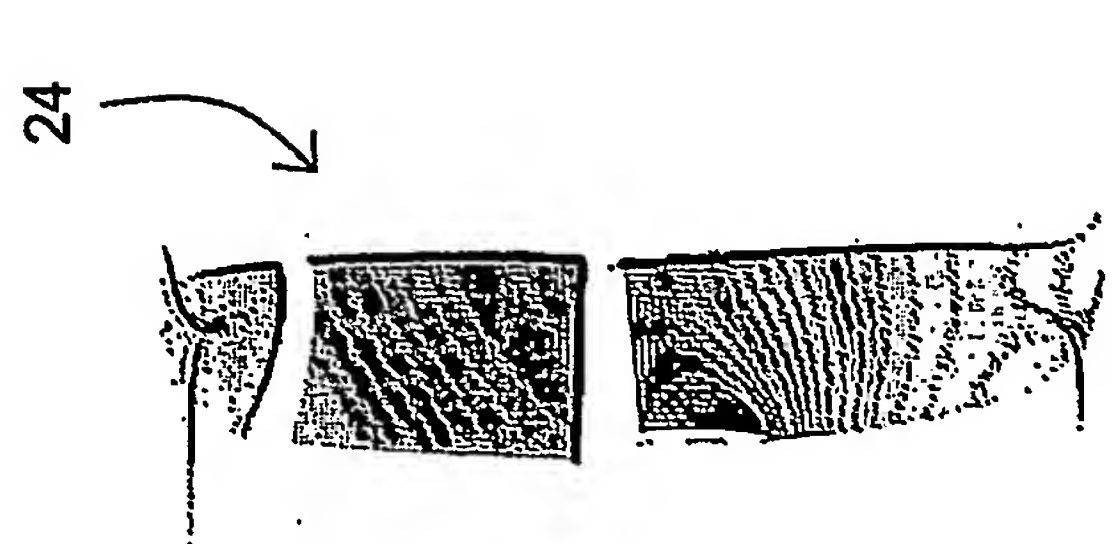

FIG 5

 Attorney's Docket No. PHUS040040USP (#899879)

APPLICATION DATA SHEET

Mail Stop: Provisional Patent Application
Commissioner for Patents
P.O. Box 1450
Alexandria, VA 22313-1450

Inventor Information

Inventor One Given Name::	Anne
Family Name::	NIEMI
City::	Helsinki
Country::	FI
Inventor Two Given Name::	Jukka
Family Name::	TANTTU
City::	Espoo
Country::	FI
Inventor Three Given Name::	Mika
Family Name::	YLIHAUTALA
City::	Vantaa
Country::	FI

Correspondence Information

Name Line One::	Thomas E. Kocovsky, Esq.
Name Line Two::	FAY, SHARPE, FAGAN,
Name Line Three::	MINNICH & McKEE, LLP
Address Line One::	1100 Superior Avenue, Seventh Floor
City::	Cleveland
State or Province::	OH
Postal or Zip Code::	44114-2518
Telephone One::	(216) 861-5582
Fax::	(216) 241-1666
Electronic Mail::	TKocovsky@faysharpe.com

Representative Information

Registration Number::	28,383

Application Information

Title Line One::	COIL SENSITIVITY ESTIMATION FOR
Title Line Two::	PARALLEL IMAGING
Total Drawing Sheets::	3
Application Type::	Provisional
Docket Number::	PHUS040040USP (#899879)

"Express Mail" Mailing Label Number EL998016713US
Date of Deposit: JANUARY 15, 2004
I hereby certify that this paper or fee is being deposited with the United States Postal Service "Express Mail Post Office to Addressee" service under 37 C.F.R. 1.10 on the date indicated above and is addressed to: Provisional Patent Application, Commissioner For Patents, P.O. Box 1450, Alexandria, VA 22313-1450.

Hilary M. McNulty
By: Hilary M. McNULTY